

# CIAS V CRP




Kanto Diagnostics



## Characteristics

- The measurement principle is Latex turbidimetric immunoassay(LTIA).
- For easily automated analyzer.
- No influence of the zone phenomenon (at least 100mg/dL).


◆◆ Calibration curve ◆◆




◆◆ Within-run precision ◆◆

Sample	1	2	3	4
N	20	20	20	20
Mean	0.071	0.411	3.283	13.980
Max	0.08	0.42	3.37	14.38
Min	0.07	0.40	3.21	13.72
Range	0.01	0.02	0.16	0.66
SD	0.002	0.004	0.042	0.155
CV (%)	2.82	0.97	1.28	1.11


◆◆ Linearity ◆◆

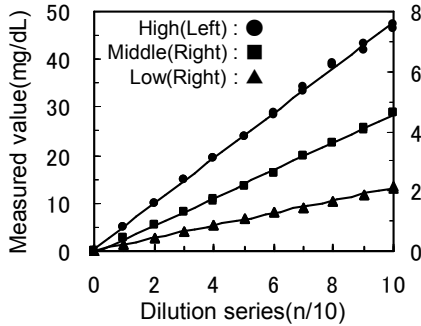


◆◆ Zone phenomenon ◆◆

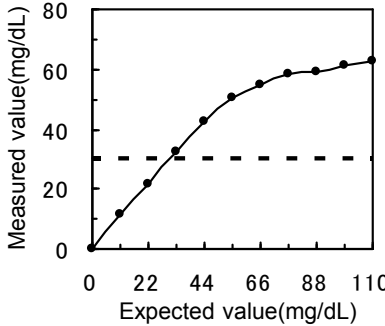



◆◆ Limit of detection ◆◆

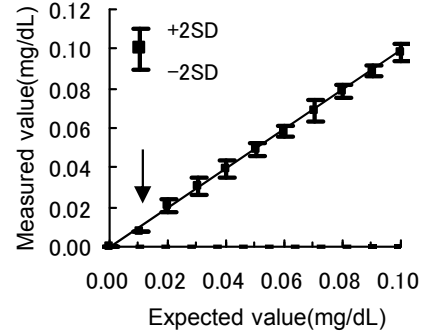

◆◆ Trueness ◆◆

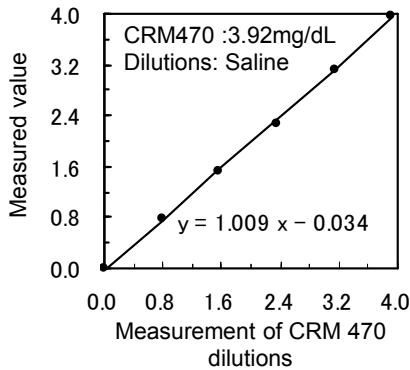


◆◆ Correlation ◆◆



◆◆ Product list ◆◆

Code	Name	Grade	Reagent	Package	Storage	Expiry
77950	Cias V CRP	7170	Reagent 1	60 mL × 3	2 - 8°C	2 years
77951			Reagent 2	60 mL × 3		
77953	V CRP Calibrator	A		1mL × 1 × 5 conc.		1 year



**Cica** **KANTO CHEMICAL CO., INC.**  
 REAGENT DIVISION  
 East Muromachi Mitsui BLDG, 2-1, Nihonbashi Muromachi 2-chome,  
 Chuo-ku, Tokyo, 103-0022 JAPAN  
 Telephone +81-3-6214-1092  
 Telefax +81-3-3241-1053  
<http://www.kanto.co.jp> E-mail:reexp-info@gms.kanto.co.jp